Method of Ultrasound Imaging

GASEOUS ULTRASOUND CONTRAST MEDIA AND
METHOD FOR SELECTING GASES FOR USE AS
ULTRASOUND CONTRAST MEDIA

draal

RELATED APPLICATIONS

This application is a continuation in part of
U.S. application Serial Number 07/893,657 filed
June 5, 1992, which is a continuation in part of U.S.
application Serial Number 07/761,311 filed
September 17, 1991.

DESCRIPTION

This invention relates to agents that enhance
the contrast in an ultrasound image generated for use
in medical diagnosis. The contrast-enhancing media
disclosed herein are comprised of extremely small gas
bubbles which are present in a solution that is
infused into the body during or just before an
ultrasound image is generated. This invention is also
directed to a method for enhancing such images by
selecting gases from which a collection of free gas
microbubbles can be prepared that have novel and
superior properties. These microbubbles, composed of
the gases whose selection is enabled by the process
of this invention, may be extremely small in size and
yet survive in the bloodstream long enough to allow
contrast-enhanced imaging of parts of the
cardiovascular system, peripheral vascular system,
and vital organs previously believed to be
inaccessible to free gas microbubbles.

BACKGROUND

When using ultrasound to obtain an image of the
internal organs and structures of a human or animal,
ultrasound waves -- waves of sound energy at a
frequency above that discernable by the human ear --

are reflected as they pass through the body.
Different types of body tissue reflect the ultrasound
waves differently and the reflections, often aptly
described as "echoes," that are produced by the
5 ultrasound waves reflecting off different internal
structures are detected and converted electronically
into a visual display. This display may prove
invaluable to a physician or other diagnostician in
several ways, including evaluating the progression of
10 cardiovascular disease or the existence or nature of
a tumor.

For some medical conditions, obtaining a useful
image of the organ or structure of interest is
especially difficult because the details of the
15 structure may not be adequately discernible from the
surrounding tissue in an ultrasound image produced by
the reflection of ultrasound waves absent a contrast-
enhancing agent. Additionally, traditional
ultrasound images are notoriously poor in quality and
20 resolution. For these reasons, detection and
observation of certain physiological conditions may
be substantially improved by enhancing the contrast
in an ultrasound image by infusing an agent into an
organ or other structure of interest. In other
25 cases, detection of the movement of the contrast-
enhancing agent itself is particularly important.
For example, a distinct blood flow pattern that is
known to result from particular cardiovascular
abnormalities may only be discernible by infusing a
30 contrasting agent into the bloodstream and observing
the dynamics of the blood flow.

Medical researchers have made extensive
investigation into the use of solids, gases and
liquids in an attempt to discover ultrasound
35 contrast-enhancing agents suitable for particular

diagnostic purposes. Composite substances such as gelatin encapsulated microbubbles, gas-incorporated liposomes, sonicated partially denatured proteins and emulsions containing highly fluorinated organic compounds have also been studied in an attempt to develop an agent that has certain ideal qualities, primarily, stability in the body and the ability to provide significantly enhanced contrast in an ultrasound image.

Small bubbles of a gas, termed "microbubbles," are readily detected in an image produced using standard ultrasound imaging techniques. When infused into the bloodstream or a particular site in the body, microbubbles enhance the contrast between the region containing the microbubbles and the surrounding tissue.

A substantial amount of the research effort directed at contrast-enhancing agents has focused on the use of extremely small gas bubbles. Investigators have long known that free gas bubbles provide a highly effective contrast agent because a gas bubble has unique physical characteristics that affect ultrasound energy as it is directed through the body. The advantages offered by free gas bubbles as opposed to liquid or solid agents that exhibit contrast enhancement is described in detail below in the context of the discussion of ultrasound diagnostic techniques.

Despite the known advantages, however, the rapid dissolution of free gas bubbles in solutions such as blood or many aqueous intravenous solutions, severely limits their use as an ultrasound contrast-enhancing agent. The most important limitations are the size of the microbubble and the length of time that a

microbubble will exist before dissolving into the solution.

Examining the size requirements for microbubbles more closely, the gas bubbles must, of course, be sufficiently small that a suspension of the bubbles does not carry the risk of embolism to the organism in which they are infused. At the same time, extremely small free gas bubbles composed of the gases generally used in ultrasound contrast imaging dissolve into solution so rapidly that their image-enhancing capability exists only immediately proximate to the infusion site. An additional obstacle exists for ultrasound imaging of the cardiovascular system. Medical researchers have studied the time required for microbubbles composed of ordinary air, pure nitrogen, pure oxygen, or carbon dioxide, to dissolve into solution. Microbubbles of these gases that are sufficiently small to be able to pass through the lungs and reach the left heart, less than about 8 microns in diameter, have a life span of less than approximately 0.25 seconds. Meltzer, R.S., Tickner, E.G., Popp, R.L., "Why Do the Lungs Clear Ultrasonic Contrast?" Ultrasound in Medicine and Biology, Vol. 6, p.263, 267 (1980). Since it takes over 2 seconds for blood to pass through the lungs, microbubbles of these gases would be fully dissolved during passage through the lungs and would never reach the left heart. Ibid. Primarily because of this tradeoff between bubble size and life span, many researchers concluded that free gas microbubbles were not useful as a contrast-enhancing agent for ultrasound diagnosis of certain parts of the cardiovascular system.

However, the ultrasound contrast-enhancing media described herein comprises microbubbles, composed of

the biocompatible gases whose selection is also provided by this invention, that are sufficiently small that they pass through the pulmonary capillary diameter of approximately 8 microns and thereby allow contrast-enhanced ultrasound diagnosis of the left chambers of the heart. The free gas microbubbles survive in the bloodstream long enough that they may be peripherally intravenously infused, travel through the right heart, through the lungs, and into the left cardiac chambers without dissolving into solution. Additionally, certain of these media have extremely long persistence in solution and will enable contrast-enhancement of many other organs and structures.

This invention overcomes many of the inherent limitations thought to exist with the use of free gas microbubbles by providing, in part, a method for selecting special gases based on particular physical criteria such that microbubbles composed of these gases do not suffer from the same limitations as the microbubbles previously investigated. Therefore, it has been discovered that the ultrasound contrast-enhancing media described herein comprising a composition of microbubbles produced using a biocompatible gas or combination of gases selected by the physical and chemical parameters disclosed herein can exist for a sufficient length of time and be of sufficiently small size that their stability in the bloodstream allows enhanced ultrasound contrast imaging of particular structures in the body previously thought inaccessible to free gas microbubbles.

By using the term "biocompatible gas" I mean a chemical entity which is capable of performing its functions within or upon a living organism in an

acceptable manner, without undue toxicity or
physiological or pharmacological effects, and which
is, at the temperature of the living organism, in a
state of matter distinguished from the solid or
5   liquid states by very low density and viscosity,
relatively great expansion and contraction with
changes in pressure and temperature, and the
spontaneous tendency to become distributed uniformly
throughout any container. The following Table
10   contains the assumed body temperatures for various
living organisms:

Organism	Rectal Temperature (degree Fahrenheit)
Swine (Sus Scrofa)	101.5-102.5
Sheep (Ovis sp.)	101-103
Rabbit (Oryctolagus cuniculus)	102-103.5
Rat (Tattus morvegicus)	99.5-100.6
Monkey (Macaca mulatta)	101-102
Mouse (Mus Musculus)	98-101
Goat (Capra hircus)	101-103
Guinea pig (Cavia porcellus)	102-104
Hamster (Mesocricetus sp.)	101-103
Ham (Homo sapiens)	98.6-100.4
Horse (Equus sp.)	101-102.5
Dog (Canin familiaris)	101-102
Baboon (Papio)	98-100
Cat (Felis catus)	101-102
Cattle (Bos taurus)	101.5-102.5
Chimpanzee (Pan)	96-100

30
Techniques For Measuring Ultrasound Contrast-Enhancement Phenomena

To more fully appreciate the subject matter of
the present invention, it is useful to describe what
is presently known about the technology of ultrasound
35   imaging and to review the search for improved
ultrasound contrast-enhancing agents in that light.
Materials that are useful as ultrasound contrast
agents operate by having an effect on ultrasound
waves as they pass through the body and are reflected

to create the image from which a medical diagnosis is made. In an attempt to develop an efficient image-contrast agent, one skilled in the art recognizes that different types of substances affect ultrasound

5   waves in different ways and to varying degrees. Moreover, certain of the effects caused by contrast-enhancing agents are more readily measured and observed than others. Thus, in selecting an ideal composition for a contrast-enhancing agent, one would

10   prefer the substance that has the most dramatic effect on the ultrasound wave as it passes through the body. Also, the effect on the ultrasound wave should be easily measured. There are three main contrast-enhancing effects which can be seen in an

15   ultrasound image: backscatter, beam attenuation, and speed of sound differential. Each of these effects will be described in turn.

A.   BACKSCATTER

When an ultrasound wave that is passing through the body encounters a structure, such as an organ or

20   other body tissue, the structure reflects a portion of the ultrasound wave. Different structures within the body reflect ultrasound energy in different ways and in varying strengths. This reflected energy is

25   detected and used to generate an image of the structures through which the ultrasound wave has passed. The term "backscatter" refers to the phenomena in which ultrasound energy is scattered back towards the source by a substance with certain

30   physical properties.

It has long been recognized that the contrast observed in an ultrasound image may be enhanced by the presence of substances known to cause a large amount of backscatter. When such a substance is

administered to a distinct part of the body, the
contrast between the ultrasound image of this part of
the body and the surrounding tissues not containing
the substance is enhanced. It is well understood

5   that, due to their physical properties, different
substances cause backscatter in varying degrees.
Accordingly, the search for contrast-enhancing agents
has focused on substances that are stable and non-
toxic and that exhibit the maximum amount of

10   backscatter.

Making certain assumptions about the way a
substance reflects ultrasound energy, mathematical
formulae have been developed that describe the
backscatter phenomenon. Working with these formulae,

15   a skilled researcher can estimate the ability of gas,
liquid, and solid contrast-enhancing agents to cause
backscatter and the degree to which a particular
substance causes measurable backscatter can be
compared with other substances based on the physical

20   characteristics known to cause the backscatter
phenomenon. As a simple example, the ability of
substance A to cause backscatter will be greater than
substance B, if, all other factors being equal,
substance A is larger than substance B. Thus, when

25   both substances are encountered by an ultrasound
wave, the larger substance scatters a greater amount
of the ultrasound wave.

The capability of a substance to cause
backscatter of ultrasound energy also depends on

30   other characteristics of the substance such as its
ability to be compressed. Of particular importance
is the dramatic increase in backscatter caused by gas
bubbles due to the bubble resonance phenomenon which
is described below. When examining different

35   substances, it is useful to compare one particular

measure of the ability of a substance to cause backscatter known as the "scattering cross-section."

The scattering cross-section of a particular substance is proportional to the radius of the scatterer, and also depends on the wavelength of the ultrasound energy and on other physical properties of the substance, J. Ophir and K. J. Parker, Contrast Agents in Diagnostic Ultrasound, Ultrasound in Medicine & Biology, vol. IS, n. 4, p. 319, 323 (1989).

The scattering cross-section of a small scatterer, a, can be determined by a known equation:

$$\sigma = \left[\frac{4}{9} \pi a^2 (ka)^4 \right] \left[\left| \frac{\kappa_s - \kappa}{\kappa} \right|^2 + \frac{1}{3} \left| \frac{3(\rho_s - \rho)}{2\rho_s - \rho} \right|^2 \right]$$

where $\kappa = 2\pi/\lambda$, where λ is the wavelength; a = the radius of the scatterer; κ_s = adiabatic compressibility of the scatterer; κ = adiabatic compressibility of the medium in which the scatterer exists, ρ_s = density of the scatterers and ρ = the density of the medium in which the scatterer exists. P. M. Morse and K. U. Ingard, Theoretical Acoustics, p. 427, McGraw Hill, New York (1968).

In evaluating the utility of different substances as image contrasting agents, one can use this equation to determine which agents will have the higher scattering cross-section and, accordingly, which agents will provide the greatest contrast in an ultrasound image.

Referring to the above equation, the first bracketed quantity in the above equation can be assumed to be constant for the purpos of comparing solid, liquid and gaseous scatterers. It can be assumed that the compressibility of a solid particle

is much less than that of the surrounding medium and
that the density of the particle is much greater.
Using this assumption, the scattering cross section
of a solid particle contrast-enhancing agent has been
5   estimated as 1.75. Ophir and Parker, supra, at 325.

For a pure liquid scatterer, the adiabatic
compressibility and density of the scatterer κ_s and
the surrounding medium κ are likely to be
approximately equal which would, from the above
10   equation, yield the result that liquids would have a
scattering cross-section of zero. However, liquids
may exhibit some backscatter if large volumes of a
liquid agent are present presumably because the term
a in the first bracketed quantity in the above
15   equation may become sufficiently large. For example,
if a liquid agent passes from a very small vessel to
a very large one such that the liquid occupies
substantially all of the vessel the liquid may
exhibit measurable backscatter. Nevertheless, in
20   light of the above equation and the following, it is
appreciated by those skilled in the art that pure
liquids are relatively inefficient scatterers
compared to free gas microbubbles.

It is known that changes in the acoustic
25   properties of a substance are pronounced at the
interface between two phases, i.e., liquid/gas,
because the reflection characteristics of an
ultrasound wave change markedly at this interface.
Additionally, the scatter cross-section of a gas is
30   substantially different than a liquid or solid, in
part, because a gas bubble can be compressed to a
much greater degree than a liquid or solid. The
physical characteristics of gas bubbles in solution
are known and standard values for compressibility and
35   density figures for ordinary air can be used in the

above equation. Using these standard values, the
result for the second bracketed term alone in the
above equation is approximately 10^{14}, Ophir and Parker
supra, at 325, with the total scattering cross

5   section varying as the radius a of the bubble varies.
Moreover, free gas bubbles in a liquid exhibit
oscillatory motion such that, at certain frequencies,
gas bubbles will resonate at a frequency near that of
the ultrasound waves commonly used in medical

10   imaging. As a result, the scattering cross-section
of a gas bubble can be over a thousand times larger
than its physical size.

Therefore, it is recognized that gas micro-
bubbles are superior scatterers of ultrasound energy

15   and would be an ideal contrast-enhancing agent if the
obstacle of their rapid dissolution into solution
could be overcome.

B.   BEAM ATTENUATION

Another effect which can be observed from the

20   presence of certain solid contrast-enhancing agents,
is the attenuation of the ultrasound wave. Image
contrast has been observed in conventional imaging
due to localized attenuation differences between
certain tissue types. K. J. Parker and R. C. Wang,

25   "Measurement of Ultrasonic Attenuation Within Regions
selected from B-Scan Images," IEEE Trans. Biomed.
Enar. BME 30(8), p. 431-37 (1983); K. J. Parker, R.
C. Wang, and R. M. Lerner, "Attenuation of Ultrasound
Magnitude and Frequency Dependence for Tissue

30   Characterization," Radiology, 153(3), p. 785-88
(1984). It has been hypothesized that measurements
of the attenuation of a region of tissue taken before
and after infusion of an agent may yield an enhanced
image. However, techniques based on attenuation

35   contrast as a means to measur the contrast

enhancement of a liquid agent are not well-developed
and, even if fully developed, may suffer from
limitations as to the internal organs or structures
with which this technique can be used. For example,
5   it is unlikely that a loss of attenuation due to
liquid contrast agents could be observed in the image
of the cardiovascular system because of the high
volume of liquid contrast agent that would need to be
present in a given vessel before a substantial
10.   difference in attenuation could be measured.

Measurement of the attenuation contrast caused
by microspheres of Albunex (Molecular Biosystems, San
Diego, CA) in vitro has been accomplished and it has
been suggested that in vivo attenuation contrast
15   measurement could be achieved. H. Bleeker, K. Shung,
J. Burnhart, "On the Application of Ultrasonic
Contrast Agents for Blood Flowometry and Assessment
of Cardiac Perfusion," J. Ultrasound Med. 9:461-471
(1990). Albunex is a suspension of 2-4 micron
20   encapsulated air-filled microspheres that have been
observed to have acceptable stability in vivo and are
sufficiently small in size that contrast enhancement
can occur in the left atrium or ventricle. Also,
attenuation contrast resulting from iodipamide ethyl
25   ester (IDE) particles accumulated in the liver has
been observed. Under such circumstances, the
contrast enhancement is believed to result from
attenuation of the ultrasound wave resulting from the
presence of dense particles in a soft medium. The
30   absorption of energy by the particles occurs by a
mechanism referred to as "relative motion." The
change in attenuation caused by relative motion can
be shown to increase linearly with particle
concentration and as the square of the density
35   difference between the particles and the surrounding

medium. K. J. Parker, et al., "A Particulate
Contrast Agent with Potential for Ultrasound Imaging
of Liver," Ultrasound in Medicine & Biology, Vol. 13,
No. 9, p. 555, 561 (1987). Therefore, where

5   substantial accumulation of solid particles occurs,
attenuation contrast may be a viable mechanism for
observing image contrast enhancement although the
effect is of much smaller magnitude than the
backscatter phenomenon and would appear to be of

10   little use in cardiovascular diagnoses.

C.   SPEED OF SOUND DIFFERENTIAL

       An additional possible technique to enhance
contrast in an ultrasound image has been proposed
based on the fact that the speed of sound varies

15   depending on the media through which it travels.
Therefore, if a large enough volume of an agent,
through which the speed of sound is different than
the surrounding tissue, can be infused into a target
area, the difference in the speed of sound through

20   the target area may be measurable. Presently, this
technique is only experimental.

       Therefore, considering the three techniques
described above for contrast enhancement in an
ultrasound image, the marked increase in backscatter

25   caused by free gas microbubbles is the most dramatic
effect and contrast-enhancing agents that take
advantage of this phenomenon would be the most
desirable if the obstacle of their limited stability
in solution could be overcome.

30   The Materials Presently Used
                     as Contrast-Enhancing Agents

       In light of what is known about the various
techniques described above, attempts to develop a
contrast-enhancing agent whose presence generates

substantial contrast in an ultrasound image, and
whose survival in vivo is sufficiently long to allow
contrast-enhanced imaging of the cardiovascular
system, has led to the investigation of a broad

5   variety of substances -- gases, liquids, solids, and
combinations of these -- as potential contrast-
enhancing agents.

A.   SOLID PARTICLES

Typically, the solid substances that have been

10   studied as potential contrast-enhancing agents are
extremely small particles that are manufactured in
uniform size. Large numbers of these particles can
be infused and circulate freely in the bloodstream or
they may be injected into a particular structure or

15   region in the body.

IDE particles are solid particles that can be
produced in large quantities with a relatively narrow
size distribution of approximately 0.5-2.0 microns.
Sterile saline injections of these particles may be

20   injected and will tend to accumulate in the liver.
Once a substantial accumulation occurs, contrast
enhancement may be exhibited by either attenuation
contrast or backscatter mechanisms. Although
suspensions comprising these solid particles

25   dispersed in a liquid may exhibit acceptable
stability, the backscatter or attenuation effects are
relatively minor compared to free gas bubbles and a
substantial accumulation of the particles must occur
before appreciable contrast is observed in an

30   ultrasound image. Thus, use of these suspensions has
been limited to certain cell types in which the
particles have the tendency to coagulate because
unless the suspension becomes highly concentrated in
particular tissue, the contrast enhancement will be

35   minor.

SHU-454 (Schering, A. G., West Berlin, Germany) is an experimental contrast-enhancing agent in powder form that, when mixed with a saccharide diluent, forms a suspension of crystals of various rhomboid and polyhedral shapes ranging in size from 5 to 10 microns. Although the precise mechanism by which these crystals enhance ultrasound contrast is not completely understood, it is suspected that the crystals may trap microbubbles in their structure or that the crystals themselves may backscatter ultrasound energy by an as-yet undetermined mechanism.

B. LIQUIDS AND EMULSIONS

In another attempt to achieve a satisfactory agent, emulsions are prepared by combining a chemical species compatible with body tissue and a species that provides high ultrasound contrast enhancement. European Patent Application 0231091 discloses emulsions of oil in water containing highly fluorinated organic compounds that have been studied in connection with their possible use as a blood substitute and are also capable of providing enhanced contrast in an ultrasound image.

Emulsions containing perfluorooctyl bromide (PFOB) have also been examined. Perfluorooctyl bromide emulsions are liquid compounds known to have the ability to transport oxygen. PFOB emulsions have exhibited a limited utility as ultrasound contrast agents because of a tendency to accumulate in certain types of cells. Although the mechanism is not completely understood, PFOB emulsions may provide ultrasound contrast because of their high density and relatively large compressibility constant.

United States Patent No. 4,900,540 describes the use of phospholipid-based liposomes containing a gas

or gas precursor as a contrast-enhancing agent. A liposome is a microscopic, spherical vesicle, containing a bilayer of phospholipids and other amphipathic molecules and an inner aqueous cavity, all of which is compatible with the cells of the body. In most applications, liposomes are used as a means to encapsulate biologically active materials. The above reference discloses the use of a gas or gas precursors incorporated into the liposome core to provide a longer life span for the gas when infused into the body. Production of stable liposomes is an expensive and time consuming process requiring specialized raw materials and equipment.

C.   MICROBUBBLES

As noted above, a critical parameter that must be satisfied by a microbubble used as a contrast-enhancing agent is size. Free gas microbubbles larger than approximately 8 microns may still be small enough to avoid impeding blood flow or occluding vascular beds. However, microbubbles larger than 8 microns are removed from the bloodstream when blood flows through the lungs. As noted above, medical researchers have reported in the medical literature that microbubbles small enough to pass through the lungs will dissolve so quickly that contrast enhancement of left heart images is not possible with a free gas microbubble. Meltzer, R.S., Tickner, E.G., Popp, R.L., "Why Do the Lungs Clear Ultrasonic Contrast?" Ultrasound in Medicine and Biology, vol. 6, p.263, 267 (1980).

However, cognizant of the advantages to be gained by use of microbubbles as contrast-enhancing agents by virtue of their large scattering cross-section, considerable attention has been focused on developing mixtures containing microbubbles that are

rendered stable in solution. Enhancing the stability
of gas microbubbles may be accomplished by a number
of techniques.

Each of the following techniques essentially
involves suspending a collection of microbubbles in a
substrate in which a bubble of ordinary gas is more
stable than in the bloodstream.

In one approach, microbubbles are created in
viscous liquids that are injected or infused into the
body while the ultrasound diagnosis is in progress.
The theory behind the use of viscous fluids involves
an attempt to reduce the rate at which the gas
dissolves into the liquid and, in so doing, provide a
more stable chemical environment for the bubbles so
that their lifetime is extended.

Several variations on this general approach have
been described. EPO Application No. 0324938
describes a viscous solution of a biocompatible
material, such as a human protein, in which
microbubbles are contained. By submitting a viscous
protein solution to sonication, microbubbles are
formed in the solution. Partial denaturation of the
protein by chemical treatment or heat provides
additional stability to microbubbles in the solution
by decreasing the surface tension between bubble and
solution.

Therefore, the above approaches may be
classified as an attempt to enhance the stability of
microbubbles by use of a stabilizing medium in which
the microbubbles are contained. However, none of
these approaches have addressed the primary physical
and chemical properties of gases which have seriously
limited the use of fr e gas microbubbles in
ultrasound diagnosis, particularly with respect to
the cardiovascular system. None of these approaches

suggest that selection of the gases, by precise criteria, would yield the ability to produce stable microbubbles at a size that would allow transpulmonary contrast-enhanced ultrasound imaging.

The behavior of microbubbles in solution can be described mathematically based on certain parameters and characteristics of the gas of which the bubble is formed and the solution in which the bubble is present. Depending on the degree to which a solution is saturated with the gas of which the microbubbles are formed, the survival time of the microbubbles can be calculated. P.S. Epstein, M.S. Plesset, "On the Stability of Gas Bubbles in Liquid-Gas Solutions," The Journal of Chemical Physics, Vol. 18, n. 11, 1505 (1950). Based on calculations, it is apparent that as the size of the bubble decreases, the surface tension between bubble and surrounding solution increases. As the surface tension increases, the rate at which the bubble dissolves into the solution increases rapidly and, therefore, the size of the bubble decreases more and more rapidly. Thus, the rate at which the bubble shrinks increases as the size of the bubble decreases. The ultimate effect of this is that a population of small free gas microbubbles composed of ordinary air dissolves so rapidly that the contrast-enhancing effect is extremely short lived. Using known mathematical formula, one can calculate that a microbubble of air that is 8 microns in diameter, which is small enough to pass through the lungs, will dissolve in between 190 and 550 milliseconds depending on the degree of saturation of the surrounding solution. Based on these calculations, medical investigators studying the way in which the lungs remove ultrasound contrast agent have calculated the dissolution times of oxygen

and nitrogen gas microbubbles in human and canine blood and have concluded that free gas microbubble contrast agents will not allow contrast-enhanced imaging of the left ventricle because of the
5   extremely brief life of the microbubbles.

     The physical properties of the systems that feature gas bubbles or gases dissolved in liquid solutions have been investigated in detail including the diffusion of air bubbles formed in the cavitating
10   flow of a liquid and the scatter of light and sound in water by gas bubbles.

     The stability of gas bubbles in liquid-gas solution has been investigated both theoretically, Epstein P.S. and Plesset M.S., On the Stability of
15   Gas Bubbles in Liquid-Gas Solutions, J. Chem. Phys. 18:1505-1509 (1950) and experimentally, Yang WJ, Dynamics of Gas Bubbles in Whole Blood and Plasma, J. Biomech 4:119-125 (1971); Yang WJ, Echigo R., Wotton DR, and Hwang JB, Experimental Studies of the
20   Dissolution of Gas Bubbles in Whole Blood and Plasma-I. Stationary Bubbles. J. Biomech 3:275-281 (1971); Yang WJ, Echigo R., Wotton DR, Hwang JB, Experimental Studies of the Dissolution of Gas Bubbles in Whole Blood and Plasma-II. Moving Bubbles or Liquids. J.
25   Biomech 4:283-288 (1971). The physical and chemical properties of the liquid and the gas determine the kinetic and thermodynamic behavior of the system. The chemical properties of the system which influence the stability of a bubble, and accordingly the life
30   time, are the rate and extent of reactions which either consume, transform, or generate gas molecules.

     For example, a well known reaction that is observed between a gas and a liquid takes place when carbon dioxide gas is present in water. As the gas
35   dissolves into the aqueous solution, carbonic acid is

created by hydration of the carbon dioxide gas. Because carbon dioxide gas is highly soluble in water, the gas diffuses rapidly into the solution and the bubble size diminishes rapidly. The presence of

5   the carbonic acid in the solution alters the acid-base chemistry of the aqueous solution and, as the chemical properties of the solution are changed by dissolution of the gas, the stability of the carbon dioxide gas bubbles changes as the solution becomes

10   saturated. In this system, the rate of dissolution of a gas bubble depends in part on the concentration of carbon dioxide gas that is already dissolved in solution.

However, depending on the particular gas or

15   liquid present in the system, the gas may be substantially insoluble in the liquid and dissolution of a gas bubble will be slower. In this situation, it has been discovered that it is possible to calculate bubble stability in a gas-liquid system by

20   examining certain physical parameters of the gas.

BRIEF DESCRIPTION OF THE INVENTION

It has been discovered that it is possible to identify chemical systems where extremely small gas bubbles are not reactive in an aqueous solution.

25   Relying on the method disclosed herein one skilled in the art may specially select particular gases based on their physical and chemical properties for use in ultrasound imaging. These gases can be used to produce the contrast-enhancing media that is also the

30   subject matter of this invention. The microbubbles can be produced using certain existing techniques that use ordinary air, and can be infused as in a conventional ultrasound diagnosis.

The method that is the subject matter of this invention requires that calculations be made, consistent with the equations provided herein, based on the intrinsic physical properties of a gas and a

5   liquid. Particularly, the density of a gas, the solubility of a gas in solution, and the diffusivity of a gas in solution, which in turn is dependent on the molar volume of the gas and the viscosity of the solution, are used in the equations disclosed below.

10   Thus, by the method disclosed herein, the physical properties of a given gas-liquid system can be evaluated, the rate and extent of bubble collapse can be estimated, and gases that would constitute effective contrast-enhancing agents can be selected

15   based on these calculations. Using existing techniques, substantially improved contrast-enhancing media may then be produced and used to improve the quality and usefulness of ultrasound imaging.

DETAILED DESCRIPTION OF THE INVENTION

20   To understand the method of this invention, it is useful to derive the mathematical relationships that describe the parameters of a gas-liquid system and the effect on bubble stability that occurs when a value for one or more of these parameters is altered.

25   It is assumed that, at an initial time, T_0, a spherical gas bubble of gas X, with a radius of R_0, is placed in a solution in which the initial concentration of gas X dissolved in the solution is equal to zero. Over some period of time, the bubble

30   of gas X will dissolve into the solvent at which time its radius R will equal zero. Assume further that the solution is at constant temperature and pressure and that the dissolved gas concentration for a solution saturated with the particular gas is

designated C_s. Thus, at T_o, the concentration of the gas in the solution is zero, meaning that none of the gas has yet dissolved and all of the gas that is present is still contained within the bubble of

5   radius R_0.

As time progresses, due to the difference in the concentration of the gas in the bubble and the gas in solution, the bubble will tend to shrink as gas in the bubble is dissolved into the liquid by the

10   process of diffusion. The change in bubble radius from its original radius of R_0 to, after the passage of a particular amount of time, a smaller radius R is expressed by Equation (1),

15

$$\frac{R}{R_0} = \left[1 - \left(\frac{2DC_s}{\rho R_0^2} \right) T \right]^{1/2}$$

where R is the bubble radius at time T, D is the coefficient of diffusivity of the particular gas in the liquid, and ρ is the density of the particular

20   gas of which the bubble is composed.

It follows that the time T required for a bubble to dissolve completely may be determined from Equation (1) by setting $R/R_0 = 0$, and solving for T:

25   Equation (2) $T = \dfrac{R_0^2 \rho}{2DC_s}$

This result qualitatively indicates that bubble stability, and hence life span, is enhanced by increasing the initial bubble size R_0 or by selecting

30   a gas of higher density ρ, lower solubility C_s in the liquid phase, or a lower coefficient of diffusivity D.

The diffusivity D of a gas in a liquid is dependent on the molar volume of the gas (Vm), and

the viscosity of the solution (η) as expressed by a known Equation;

(Equation 3) $D = 13.26 \times 10^{-5} \cdot \eta^{-1.14} \cdot V_m^{-0.589}$

By substituting the expression for D given in Equation (3) into Equation (2) it is revealed that bubble stability is enhanced by using gases of larger molar volume Vm, which tend to have a higher molecular weight, and liquids of higher viscosity.

By way of example, a comparison of the stability of air microbubbles and microbubbles composed of gases specially selected by the method disclosed herein may be made. Taking the value of D for air in water at 22°C as 2×10^{-5} $cm^2 sec^{-1}$ and the ratio $C_s/\rho = 0.02$ (Epstein and Plesset, Ibid.), one obtains the following data for the time t for complete solution of air bubbles in water (unsaturated with air) :

TABLE I

INITIAL BUBBLE DIAMETER, microns	TIME, milliseconds
12	450
10	313
8	200
6	113
5	78
4	50
3	28
2	13
1	3

If the blood transit time from the pulmonary capillaries to the left ventricle is two seconds or more (Hamilton, W.F. editor, Handbook of Physiology, Vol. 2, section 2, CIRCULATION. American Physiology Society, Washington, D.C., p. 709, (1963)), and recognizing that only microbubbles of approximately 8 microns or less will be small enough to pass through the lungs, it is clear that none of these bubbles

have a life span in solution long enough to be useful contrast agents for ultrasound contrast-enhanced imaging of the left ventricle.

5   The method of the present invention allows identification of potentially useful gases by comparing the properties of any particular gas, denoted gas X in the following description, to air. Taking Equations (2) and (3) above, a coefficient Q may be formulated for a particular gas X that will

10   describe the stability of microbubbles composed of gas X in a given liquid. The value of the Q coefficient determined by this method for a particular gas X also can be used to determine the utility of gas X as an ultrasound contrast-enhancing

15   agent as compared to ordinary air.

From Equation (2) above, an equation that describes the time for complete dissolution of a bubble of gas X compared to the same size bubble of ordinary air under identical conditions of solution

20   temperature and solution viscosity may be written based on the physical properties of gas X and air:
Equation (4)

25
$$T_x = T_{air} \left[\frac{\rho_x}{\rho_{air}} \right] \left[\frac{(C_s)_{air}}{(C_s)_x} \right] \left[\frac{D_{air}}{13.26 \times 10^{-5} \cdot \eta^{-1.14} \cdot (V_m)_x^{-.589}} \right]$$

or, if D is known for gas X,
Equation (5)

30
$$T_x = T_{air} \left[\frac{\rho_x}{\rho_{air}} \right] \left[\frac{(C_s)_{air}}{(C_s)_x} \right] \left[\frac{D_{air}}{D_x} \right]$$

To formulate this equation so that the value Q may be obtained to enable comparison of gas X with air, the above equation may be rewritten:

Equation (6) $T_x = QT_{air}$ where

$$Q = \left[\frac{\rho_x}{\rho_{air}} \right] \left[\frac{(C_s)_{air}}{(C_s)_x} \right] \left[\frac{D_{air}}{D_x} \right]$$

Assuming for comparison, a solution of water at 22 degrees C, the density, diffusivity, and solubility of air in the solution are known quantities which may be substituted into the above equation yielding:

Equation (7) $Q = 4.0 \times 10^{-7} \left[\frac{\rho_x}{(C_x)_x D_x} \right]$

Substituting Equation (3) into the above for gases whose diffusivity D_x is not readily known, and assuming that the viscosity term η below for water at 22 degrees C is approximately equal to 1.0 cP,

Equation (8) $Q = 3.0 \times 10^{-3} \left[\frac{\rho_x}{(C_s)_x (V_m)_x^{-.589}} \right]$

Thus, knowing the density, solubility and molar volume of a gas, this method allows the calculation of the value of the Q coefficient.

If Q is less than one, microbubbles of gas X will be less stable in a given solvent than microbubbles of air. If Q is greater than one, microbubbles formed of gas X are more stable than microbubbles of air and will survive in solution longer than air bubbles. All other properties being the same for a given microbubble size, the time for complete dissolution of a microbubble of gas X is equal to the time for comple te dissolution of a microbubble of ordinary air multiplied by the Q

coefficient. For example, if the Q coefficient for
gas X is 10,000, a microbubble of gas X will survive
10,000 times as long in solution compared to a
microbubble of air. A Q value can be determined for
5   any gas in any solution assuming the quantities
identified herein are known or can be estimated.

Different methods for determining or estimating
values for the individual parameters of density,
diffusivity, and solubility may be needed depending
10   on the chemical structure of the gas. Values for
these parameters may or may not be available from
known scientific literature sources such as the *Gas
Encyclopedia* or the tabulations published by the
American Chemical Society. Values for the density of
15   most gases are readily available from sources such as
the Handbook of Chemistry and Physics, CRC Press, 72d
Ed. (1991-92). Additionally, the solubility in water
and molar volume of some gases has been measured with
accuracy. In many cases however, calculations for
20   the numerical values for molar volume and solubility
may need to be calculated or estimated to provide the
data used to determine the value of the Q coefficient
for an individual gas by the method described above.
An example of the calculation of Q values for a
25   preferred selection of gases illustrates how the
method of this invention can be applied to individual
gases.

Generally, many fluorine-containing gases
exhibit extremely low solubility in water, and have
30   relatively high molecular weights, high molar
volumes, and high densities. To determine the Q
value for several gases, the solubility, molar volume
and density of the individual gases are determined
and the values are substituted into Equations (7) or
35   (8) above.

Determination of Gas Solubility for Fluorocarbons

This method for estimating the gas solubility of fluorocarbons uses extrapolation of the experimental data of Kabalnov AS, Makarov KN, and Scherbakova OV. "Solubility of Fluorocarbons in Water as a Key Parameter Determining Fluorocarbon Emulsion Stability," J. Fluor. Chem. 50, 271-284, (1990). The gas solubility of these fluorocarbons is determined relative to perfluoro-n-pentane which has a water solubility of 4.0×10^{-6} moles per liter. For a homologous series of non-branched fluorocarbons, the gas solubility may be estimated by increasing or reducing this value by a factor of about 8.0 for each increase or reduction in the number of additional $-CF_2-$ groups present in the molecule.

Determination of Molar Volume

The molar volume (Vm) is estimated from the data of Bondi A., "Van der Waals Volumes and Radii," J. Phys. Chem. 68, 441-451 (1964). The molar volume of a gas can be estimated by identifying the number and type of atoms that make up the molecule of gas in question. By determining the number and type of atoms present in the molecule and how the individual atoms are bound to each other, known values may be applied for the molecular volume of the individual atoms. By considering the contribution of each individual atom and its frequency of occurrence, one may calculate the total molar volume for a particular gas molecule. This calculation is best demonstrated with an example.

It is known that a carbon molecule in an alkane carbon-carbon bond has a molar volume of 3.3 cubic centimeters per mole, a carbon atom in an alkene

carbon-carbon bond has a molar volume of 10.0 cubic centimeters per mole, and when multiple fluorine atoms are bound to an alkane carbon, a fluorine atom has a molar volume of 6.0 cubic centimeters per mole.

5   Examining octafluoropropane, this molecule contains three carbon atoms in alkane carbon-carbon bonds (3 atoms at 3.3 cubic centimeters per mole) and 6 fluorine atoms bound to alkane carbons (6 atoms at 6.0 cubic centimeters per mole) hence, octafluoro-

10   propane has a molar density of 58 cubic centimeters per mole.

Once density, molar volume, and solubility are determined, the Q value is calculated using Equation 8 above.

15   The following Table lists the Q value for a number of gases based on the calculations detailed above.

TABLE II

GAS	DENSITY	SOLUBILITY	MOLAR VOLUME	Q
	kg/m3	micromoles/ liter	cm3/mole	
Argon	1.78	1500	17.9	20
n-Butane	2.05	6696	116	5
Carbon Dioxide	1.98	33000	19.7	1
Decafluorobutane	11.21	32	73	13,154
Dodecafluoropentane	12.86	4	183	207,437
Ethane	1.05	2900	67	13
Ethyl ether	2.55	977,058	103	0.1
Helium	0.18	388	8	5
Hexafluorobuta-1,3-diene	9 (*)	2000	56	145
Hexafluoro-2-butyne	9 (*)	2000	58	148
Hexafluoroethane	8.86	2100	43	116
Hexafluoropropane	10.3	260	58	1299
Krypton	3.8	2067	35	44
Neon	0.90	434	17	33
Nitrogen	##	##	##	1
Octafluoro-2-butene	10 (*)	220	65	1594
Octafluorocyclobutane	9.97	220	61	1531
Octafluoropropane	10.3	260	58	1299
Pentane	2	1674	113	58

Propane	2.02	2902	90	30
Sulfur Hexafluoride	5.48	220	47	722
Xenon	5.90	3448	18	28

* These density values are estimated from the known density of homologous fluorocarbons.

The solubility/density ratio value of 0.02 (supra) and the diffusivity of 2×10^{-5} cm^{2}sec-1 given above were used in equation 7 for this Q-value determination.

Once the Q value has been determined the utility of an individual gas as an ultrasound contrast-enhancing agent can be analyzed by determining the life span of a collection of microbubbles composed of the gas in question at different sizes, as was done for air in Table I above. Taking the value of Q for decafluorobutane and examining the time necessary for various sized bubbles to dissolve in water, one obtains the values in Table III below by multiplying each of the time values in Table I by the Q value for decafluorobutane:

TABLE III

INITIAL BUBBLE DIAMETER, microns	TIME, minutes
12	99
10	69
8	44
6	25
5	17
4	11
3	6.1
2	2.9
1	0.7

Notice that the time scale in Table III is minutes rather than milliseconds as was the case for air. All bubbles of decafluorobutane, even as small as 1 micron, can be injected peripherally and will not dissolve into solution during the approximately 10 seconds needed to reach the left ventricle. Similar calculations can be performed for a gas with any Q coefficient. Slightly larger bubbles will be

able to pass through the lungs and yet survive long enough to permit both examination of myocardial perfusion and dynamic abdominal organ imaging. Moreover, as with many of the gases identified by

5   this method, decafluorobutane features low toxicity at small dosages and would, therefore, offer substantial advantages as a contrast-enhancing agent in conventional ultrasound diagnosis.

Manual creation of a microbubble suspension may

10   be accomplished by several methods. United States Patent 4,832,941, the disclosure of which is incorporated herein by reference, refers to a method for producing a suspension of microbubbles with a diameter less than seven microns created by spraying

15   a liquid through a quantity of gas using a three-way tap. Although techniques could vary in practice, the three-way tap is a preferred method to manually suspend a quantity of high Q coefficient gas to produce the contrast-enhancing media described

20   herein.

The general techniques for use of a three-way tap device are well known in connection with preparation of the common Freund's adjuvant for immunizing research animals. Typically, a three-way

25   tap is comprised of a pair of syringes, both of which are connected to a chamber. The chamber has outlet from which the suspension may be collected or infused directly.

Techniques for use of the three-way tap may

30   differ from that described in U.S. Patent No. 4,832,941 because different gases are being used in this procedure. For example, use of one of the high Q coefficient gases disclosed herein may be more efficient if the system is purged of ordinary air or

flushed with another gas before the microbubble
suspension is produced.

In a preferred embodiment of the present
invention, a 40-50% Sorbitol (D-glucitol) solution is
5   mixed with approximately 1-10% by volume of a high Q-
coefficient gas with approximately 5% gas being an
optimal value. Sorbitol is a commercially available
compound that when mixed in an aqueous solution
substantially increases the viscosity of the
10   solution. Higher viscosity solutions, as seen in
equation 3 above, extend the life of a microbubble in
solution. A 40-50% Sorbitol solution is preferred to
maintain as a bolus upon injection; that is as intact
as possible without exceeding a tolerable injection
15   pressure. To produce the suspension of microbubbles,
a quantity of the chosen gas is collected in a
syringe. In the same syringe, a volume of the
Sorbitol solution may be contained. A quantity of
Sorbitol solution is drawn into the other syringe so
20   that the sum of the two volumes yields the proper
percentage of gas based on the volume percentage of
microbubbles desired. Using the two syringes, each
featuring a very small aperture, the liquid is
sprayed into the gas atmosphere approximately 25
25   times or as many times as is necessary to create a
suspension of microbubbles whose size distribution is
acceptable for the purposes described herein. This
technique may be varied slightly, of course, in any
manner that achieves the resulting suspension of
30   microbubbles of the desired size in a desired
concentration. Microbubble size may be checked
either visually or electronically using a Coulter
Counter (Coulter Electronics) by a known method,
Butler, B.D., "Production of Microbubble for Use as

Echo Contrast Agents," J. Clin. Ultrasound, V.14 408
(1986).

EXAMPLES

EXAMPLE 1. An ultrasound contrast agent was prepared
using decafluorobutane as the microbubble-forming
gas. A solution was prepared containing:

sorbitol	20.0 g
NaCl	0.9 g
soy bean oil	6.0 mL
Tween 20	0.5 mL
water q.s.	100.0 mL

A soapy, clear, yellow solution was afforded
with stirring. A 10 mL aliquot of this solution was
taken up in a 10 mL glass syringe. The syringe was
then attached to a three-way stopcock. A second 10
mL syringe was attached to the stopcock and 1.0 cc of
decafluorobutane (PCR, Inc., Gainesville, FL) was
delivered to the empty syringe. The stopcock valve
was opened to the solution-containing syringe and the
liquid and gas phases mixed rapidly 20-30 times. A
resulting milky-white, slightly viscous solution was
obtained.

EXAMPLE 2. The gas emulsion obtained in Example 1
was diluted with water (1:10 to 1:1000), placed in a
hemocytometer, and examined under the microscope
using an oil immersion lens. The emulsion consisted
of predominately 2-5 micron bubbles. The density was
50-100 million microbubbles per mL of original
undiluted formulation.

EXAMPLE 3. The formulation of Example 1 was prepared
and echocardiography performed in a canine model. A
17.5 kg mongrel dog was anesthetized with isoflurane
and monitors established to measure ECG, blood

pressure, heart rate, and arterial blood gases according to the methods described by Keller, MW, Feinstein, SB, Watson, DD: Successful left ventricular opacification following peripheral venous injection of sonicated contrast agent: An experimental evaluation. Am Heart J 114:570d (1987).

The results of the safety evaluation are as follows:

MAXIMUM PERCENTAGE CHANGE IN MEASURED PARAMETER WITHIN 5 MIN POST INJECTION

DOSE	AORTIC PRESSURE			BLOOD GASES			HEART RATE	
	SYSTOLIC mm Hg	DIASTOLIC	MEAN	PaO2	PaCO2	pH		
0.5 mL	+6, -14	+9, 0	+8, -6	329	58.1	7.26	+10	-19
1.0 mL	+9, -2	+5, -1	+4, -4				+1,	-4
2.0 mL	+5, -3	+5, -1	+5, -1				0,	-1
3.0 mL	+6, -2	+7, 0	+4, -3				0,	-3
4.0 mL	+5, -1	+3, -3	+5, -3				0,	-3
5.0 mL	0, -10	+1, -3	0, -4				+1,	-1
7.0 mL	0, -13	0, -8	0, -9	313	28.6	7.36	0,	-1

All changes were transient and returned to baseline values typically within 3-6 minutes. The above safety data demonstrate minimal changes in the measured hemodynamic parameter. All doses provided both right and left ventricular chamber opacification. The intensity increased with the increasing dose.

Example 4. The above specific determinations of the suitability of a particular gas for use as an ultrasound agent can be approximated if the molecular weight of a particular gas is known, can be calculated, or can be measured. This approximation is based on the determination that there is a linear relationship

between the logarithm of the Q-value and the molecular weight for a gas, as shown in the Figure below.
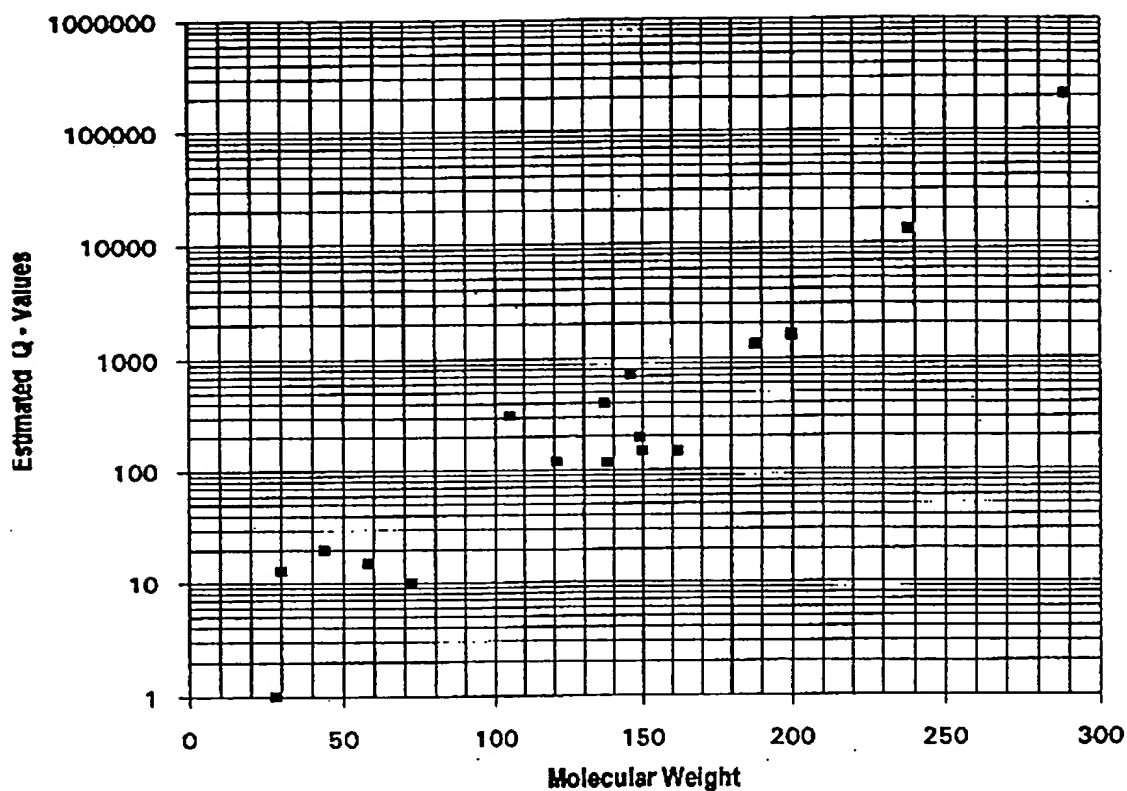
Based on this Figure, the following guidelines can be used to estimate a Q-value:

Molecular Weight	Estimated Q-Value
< 35	< 5
35-70	5-20
71-100	21-80
101-170	81-1000
171-220	1001-10,000
221-270	10,001-100,000
>270	>100,000

The following Table contains a series of gases with the relevant data on molecular weight and estimated Q-value. The higher the Q-value the more

promising is the particular gas. Especially promising are gases with Q-values greater than five. Additional issues, including, but not limited to, cost and toxicity, should be considered in addition to longevity of the derived microbubbles (as estimated by the Q-value) in determining the suitability of any particular gas as an ultrasound contrast agent.

TABLE IV

Chemical Name	Molecular Weight	Estimated Q Value
Acetone, hexafluoro	166.02	81-1000
Acetylene, isopropyl	68	5-20
Air	28.4	<5
Allene	40.06	5-20
Allene, tetrafluoro	112.03	81-1000
Argon	39.98	5-20
Borne, dimethyl, methoxy	71.19	21-80
Borne, trimethyl	55.91	5-20
Boron fluoride dihydrate	103.84	81-1000
1,2-Butadiene	54.09	5-20
1,3-Butadiene	54.09	5-20
1,3-Butadiene, 1,2,3-trichloro	157.43	81-1000
1,3-Butadiene, 2-fluoro	72.08	21-80
1,3-Butadiene, 2-methyl	68.12	5-20
1,3-Butadiene, hexafluoro	162.03	81-1000
Butadiyne	50.06	5-20
n-Butane	58.12	5-20
Butane, 1-fluoro	76.11	21-80
Butane, 2-methyl	72.15	21-80
Butane, decafluoro	238.03	10,001-100,000
1-Butene	56.11	5-20
2-Butene {cis}	56.11	5-20
2-Butene {trans}	56.11	5-20
1-Butene, 2-methyl	70.13	5-20
1-Butene, 3-methyl	70.13	5-20
2-Butene, 3-methyl	68	5-20
1-Butene, perfluoro	200.03	1001-10,000
2-Butene, perfluoro	200.03	1001-10,000
3-Butene-2-one, 4-phenyl {trans}	146.19	81-1000
1-Butene-3-yne, 2-methyl	66.1	5-20
Butyl nitrite	103.12	81-100
1-Butyne	54.09	5-20
2-Butyne	54.09	5-20
Butyne, 2-chloro-1,1,1,4,4,4-hexafluoro	199	1001-10,000
1-Butyne, 3-methyl	68.12	5-20
2-Butyne, perfluoro	162.03	81-1000
Butyraldehyde, 2-bromo	151	81-1000
Carbon dioxide	44.01	5-20
Carbonyl sulfide	60.08	5-20
Crotononitrile	67.09	5-20

	Cyclobutane	56.11	5-20
	Cyclobutane, methyl	70.13	5-20
	Cyclobutane, octafluoro	200.03	1001-100,000
	Cyclobutene, perfluoro	162.03	81-1000
5	Cyclopentene, 3-chloro	102.56	81-1000
	Cyclopropane	42.08	5-20
	Cyclopropane, 1,2-dimethyl {trans, dl}	70.13	5-20
	Cyclopropane, 1,1-dimethyl	70.13	5-20
	Cyclopropane, 1,2-dimethyl {cis}	70.13	5-20
10	Cyclopropane, 1,2-dimethyl {trans, l}	70.13	5-20
	Cyclopropane, ethyl	70.13	5-20
	Cyclopropane, methyl	56.11	5-20
	Deuterium	4.02	<5
	Diacetylene	50.08	5-20
15	Diaziridine, 3-ethyl-3-methyl	86.14	21-80
	Diazoethane, 1,1,1-trifluoro	110.04	81-1000
	Dimethyl amine	45.08	5-20
	Dimethyl amine, hexafluoro	153.03	81-1000
	Dimethyl disulfide, hexafluoro	202.13	1001-10,000
20	Dimethylethylamine	73.14	21-80
	bis-(Dimethyl phosphino) amine	137.1	81-1000
	2,3-Dimethyl-2-norbornano	140.23	81-1000
	Dimethylamine, perfluoro	171.02	1001-10,000
	Dimethyloxonium chloride	82.53	21-80
25	1,3-Dioxolane-2-one, 4-methyl	102.09	81-1000
	Ethane	30.07	<5
	Ethane, 1,1,1,2-tetrafluoro	102.03	81-1000
	Ethane, 1,1,1-trifluoro	84.04	21-80
	Ethane, 1,1,2,2-tetrafluoro	102.03	81-1000
30	Ethane, 1,1,2-trichloro-1,2,2-trifluoro	187.38	1001-10,000
	Ethane, 1,1-dichloro	98	21-80
	Ethane, 1,1-dichloro-1,2,2,2-tetrafluoro	170.92	1001-10,000
	Ethane, 1,1-dichloro-1-fluoro	116.95	81-1000
	Ethane, 1,1-difluoro	66.05	5-20
35	Ethane, 1,2-dichloro-1,1,2,2-tetrafluoro	170.92	1001-10,000
	Ethane, 1,2-difluoro	66.05	5-20
	Ethane, 1-chloro-1,1,2,2,2-pentafluoro	154.47	81-1000
	Ethane, 1-chloro-1,1,2,2-tetrafluoro	136.48	81-1000
	Ethane, 2-chloro, 1,1-difluoro	100	21-80
40	Ethane, 2-chloro-1,1,1-trifluoro	118.49	81-1000
	Ethane, Chloro	64.51	5-20
	Ethane, chloro pentafluoro	154.47	81-1000
	Ethane, dichlorotrifluoro	152	81-1000
	Ethane, fluoro	48.06	5-20
45	Ethane,hexafluoro	138.01	81-1000
	Ethane, nitro-pentafluoro	165.02	81-1000
	Ethane, nitroso-pentafluoro	149.02	81-1000
	Ethane, perfluoro	138.01	81-1000
	Ethyl amine, perfluoro	171.02	1001-100,000
50	Ethyl ether	74.12	21-80
	Ethyl methyl ether	60.1	5-20
	Ethyl vinyl ether	72.11	21-80
	Ethylene	28.05	<5
	Ethylene, 1,1-dichloro	96.94	21-80
55	Ethylene, 1,1-dichloro-2-fluoro	114.93	81-1000
	Ethylene, 1,2-dichloro-1,2-difluoro	132.92	81-1000
	Ethylene, 1,2-difluoro	64	5-20

	Ethylene, 1-chloro-1,2,2-trifluoro	116.47	81-1000
	Ethylene, chloro trifluoro	116.47	81-1000
	Ethylene, dichloro difluoro	132.92	81-1000
	Ethylene, tetrafluoro	100.02	21-80
5	Fulvene	78.11	21-80
	Helium	4	<5
	1,5-Heptadiyne	92.14	21-80
	Hydrogen (H2)	2.02	<5
	Isobutane	58.12	5-20
10	Isobutane, 1,2-epoxy-3-chloro	106.55	81-1000
	Isobutylene	56.11	5-20
	Isoprene	68.12	5-20
	Krypton	83.8	21-80
	Methane	16.04	<5
15	Methane sulfonyl chloride, trifluoro	168.52	81-1000
	Methane sulfonyl fluoride, trifluoro	152.06	81-1000
	Methane, (pentafluorothio)trifluoro	196.06	1001-10,000
	Methane, bromo difluoro nitroso	159.92	81-1000
	Methane, bromo fluoro	112.93	81-1000
20	Methane, bromo-chloro-fluoro	147.37	81-1000
	Methane, bromo-trifluoro	148.91	81-1000
	Methane, chloro difluoro nitro	131.47	81-1000
	Methane, chloro dinitro	140.48	81-1000
	Methane, chloro fluoro	68.48	5-20
25	Methane, chloro trifluoro	104.46	81-1000
	Methane, chloro-difluoro	86.47	21-80
	Methane, dibromo difluoro	209.82	1001-10,000
	Methane, dichloro difluoro	120.91	81-1000
	Methane, dichloro-fluoro	102.92	81-1000
30	Methane, difluoro	52.02	5-20
	Methane, difluoro-iodo	177.92	1001-10,000
	Methane, disilano	76.25	21-80
	Methane, fluoro	34.03	<5
	Methane, iodo-	141.94	81-1000
35	Methane, iodo-trifluoro	195.91	1001-10,000
	Methane, nitro-trifluoro	115.01	81-1000
	Methane, nitroso-trifluoro	99.01	21-80
	Methane, tetrafluoro	88	21-80
	Methane, trichlorofluoro	137.37	81-1000
40	Methane, trifluoro	70.01	5-20
	Methanesulfenylchloride, trifluoro	136.52	81-1000
	2-Methyl butane	72.15	21-80
	Methyl ether	46.07	5-20
	Methyl isopropyl ether	74.12	21-80
45	Methyl nitrite	61.04	5-20
	Methyl sulfide	62.13	5-20
	Methyl vinyl ether	58.08	5-20
	Neon	20.18	<5
	Neopentane	72.15	21-80
50	Nitrogen (N2)	28.01	<5
	Nitrous oxide	44.01	5-20
	1,2,3-Nonadecane tricarboxylic acid, 2-.....hydroxytrimethylester	500.72	>100,000
	1-Nonene-3-yne	122.21	81-1000
55	Oxygen (O2)	32	<5
	1,4-Pentadiene	68.12	5-20
	n-Pentane	72.15	21-80

Pentane, perfluoro	288.04	>100,000
2-Pentanone, 4-amino-4-methyl	115.18	81-1000
1-Pentene	70.13	5-20
2-Pentene {cis}	70.13	5-20
2-Pentene {trans}	70.13	5-20
1-Pentene, 3-bromo	149.03	81-1000
1-Pentene, perfluoro	250.04	10,001-100,000
Phthalic acid, tetrachloro	303.91	>100,000
Piperidine, 2,3,6-trimethyl	127.23	81-1000
Propane	44.1	5-20
Propane, 1,1,1,2,2,3-hexafluoro	152.04	81-1000
Propane, 1,2-epoxy	58.08	5-20
Propane, 2,2-difluoro	80.08	21-80
Propane, 2-amino	59.11	5-20
Propane, 2-chloro	78.54	21-80
Propane, heptafluoro-1-nitro	215.03	1001-10,000
Propane, heptafluoro-1-nitroso	199.03	1001-10,000
Propane, perfluoro	188.02	1001-10,000
Propene	42.08	5-20
Propyl, 1,1,1,2,3,3-hexafluoro-2,3-dichloro	221	10,001-100,000
Propylene, 1-chloro	76.53	21-80
Propylene, 1-chloro-{trans}	76.53	5-20
Propylene, 2-chloro	76.53	5-20
Propylene, 3-fluoro	60.07	5-20
Propylene, perfluoro	150.02	81-1000
Propyne	40.06	5-20
Propyne, 3,3,3-trifluoro	94.04	21-80
Styrene, 3-fluoro	122.14	81-1000
Sulfur hexafluoride	146.05	81-1000
Sulfur (di),decafluoro(S2F10)	298	>100,000
Toluene, 2,4-diamino	122.17	81-1000
Trifluoroacetonitrile	95.02	21-80
Trifluoromethyl peroxide	170.01	81-1000
Trifluoromethyl sulfide	170.07	81-1000
Tungsten hexafluoride	298	>100,000
Vinyl acetylene	52.08	5-20
Vinyl ether	70	5-20
Xenon	131.29	81-1000

Example 5. The relationship between a calculated Q-value for a given gas and the persistence of microbubbles of that gas was studied to determine what Q-value would be a lower limit for utility as an ultrasound contrast agent. For these experiments, a 190 x 100 mm Pyrex™ (No. 3140) evaporation dish was filled with approximately 2000 mL of water at 37°C. Five mL of a 20% sorbitol solution was taken up in a 10 mL syringe connected to a three way stopcock. A 10 mL syringe, containing 2 cubic centimeters of the subject gas (or low boiling

liquid, as pertinent) was attached to the syringe containing the sorbitol solution. The sorbitol and gas or liquid are rapidly mixed 25-times to create a suspension of microbubbles or dispersed liquid and then rapidly added to the water. The microbubbles of this method are generally about 100 microns in size, and if composed of air would have a calculated persistence of 31 sec (0.5 min). Ultrasound scans before, during and after the addition were made with a Hewlett-Packard Model Sonos 500 ultrasound scanner operating at 5 MHz. The time during which the microbubbles could be observed was recorded. The results are contained in Table V below. The experimental Q-values were obtained by dividing the measured persistence of a given gas by the measured persistence for air.

TABLE V

RELATIONSHIP BETWEEN Q-VALUE FOR A GAS AND THE PERSISTENCE OF MICROBUBBLES

GAS	Q-VALUE (Calculated)	PERSISTENCE (Experimental Q-Value)
Diethyl ether	0.1	0.1 min (0.2)
Air	1	0.6 min (1.0)
Butane	5	1.5 min (2.6)
Helium	5	2.0 min (3.5)
Propane	30	3.2 min (6.0)
Pentane	58	20.6 min (36)
Dodecafluoropentane	207,437	>5760 min (>10,105)

These experiments indicate an excellent agreement between the calculated Q-value and the experimentally determined values. Based on these data, gases with Q-values calculated to be greater than five should be potentially useful as contrast agents for ultrasound imaging.

Example 6. The relationship of the state of matter of a given chemical entity with a high Q-

coefficient and its utility as an ultrasound contrast agent was tested by comparing the efficiency of perfluoropentane and perfluorohexane to act as an ultrasound contrast agent. Perfluoropentane (dodecafluoropentane) has a calculated Q-coefficient of 207,437 and a boiling point under standard pressure conditions of 29.5 degrees Centigrade. Perfluorohexane (PCR, INc., Gainsville, FL) has a calculated Q-coefficient of 1,659,496 and a boiling point under standard pressure conditions of 59-60 degrees C. Therefore, at 37 degrees C, the body temperature of man, perfluoropentane is a gas while perfluorohexane is a liquid.

Aqueous dispersions of perfluoropentane and perfluorohexane (2% w/v) were formed at 4 degrees C by vigorous homogenization. A plastic beaker, containing approximately 1000 mL of water at 37 degrees C, was prepared to simulate human blood and was ultrasonically-scanned, as indicated in Example 5 above, before and after the addition of samples of each of the above dispersions.

Less than 1.0 mL of the perfluoropentane dispersion, when mixed with the simulated blood, produced an extremely bright ultrasound signal which persisted for at least 30 minutes. A 1:10,000 dilution was still detectable.

In contrast, a 1.0 mL sample of the perfluorohexane dispersion was undetectable by ultrasound scanning under the same conditions, as was even a 10 mL sample (1:100 dilution).

The conclusion to be drawn is that both a high Q-coefficient and a gaseous state at the body temperature of the organism being scanned is necessary for a substance to be effective as an

ultrasound contrast agent according to the method
that is the subject matter of this invention.

Although the invention has been described in
some respects with reference to specified preferred
5   embodiments thereof, variations and modifications
will become apparent to those skilled in the art. It
is, therefore, the intention that the following
claims not be given a restrictive interpretation but
should be viewed to encompass variations and
10   modifications that are derived from the inventive
subject matter disclosed. In this regard the
invention allows those skilled in the art to
determine the suitability of various chemicals as
ultrasound contrast agents where density, solubility
15   and molar volume data are available.